

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010

Graduated cylinder, 100:1,0 ml, A, conf. cert.




Batch: 47-23

Serial:

Measuring Nr. 65415

Batch size: 1199

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	19,9554 ml	60,0479 ml	100,0308 ml
Deviation:	0,1064 ml	0,0903 ml	0,0810 ml
Precision (CV):	0,5321 %	0,1505 %	0,0810 %

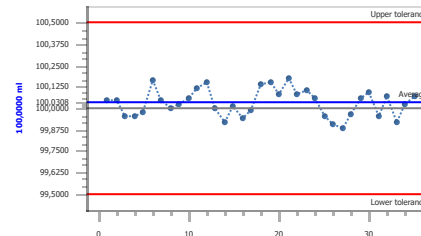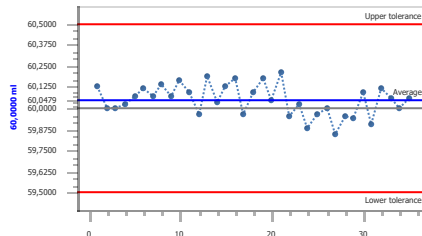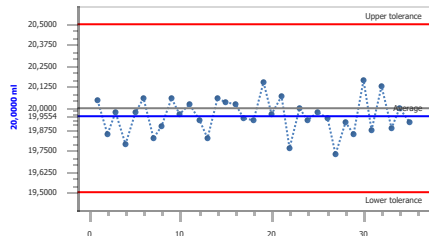

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	01.12.2023
Balance:	Sartorius - LE244S-OCE

