

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 025 USP

**Graduated cylinders, 250:2 ml, A, USP, conf. cert.**




**Batch:** 19-21

**Serial:**

**Measuring Nr.:** 46910

**Batch size:** 150

Volume:	50,000 ml	150,000 ml	250,000 ml
<b>Tolerance:</b>	± 1,000 ml	± 1,000 ml	± 1,000 ml
<b>Average value:</b>	49,7520 ml	150,0268 ml	250,1742 ml
<b>Deviation:</b>	0,2063 ml	0,1058 ml	0,1173 ml
<b>Precision (CV):</b>	0,4127 %	0,0706 %	0,0469 %

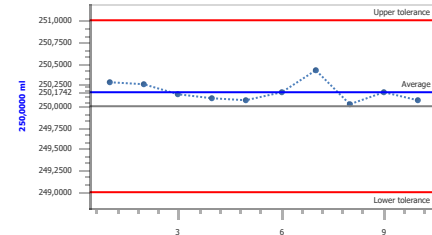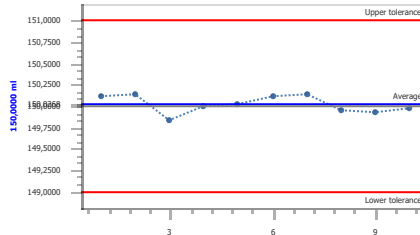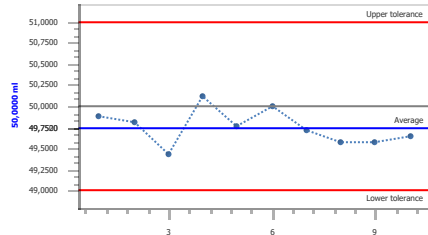

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	25.05.2021
<b>Balance:</b>	Sartorius - LA 1200 S

