

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 025

Graduated cylinders, 250:2 ml, A, conf. cert.




Batch: 24-18

Serial:

Measuring Nr.: 21690

Batch size: 500

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
Average value:	50,0638 ml	149,9943 ml	249,9400 ml
Deviation:	0,2074 ml	0,1434 ml	0,1559 ml
Precision (CV):	0,4148 %	0,0956 %	0,0623 %

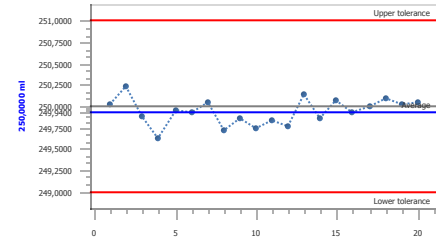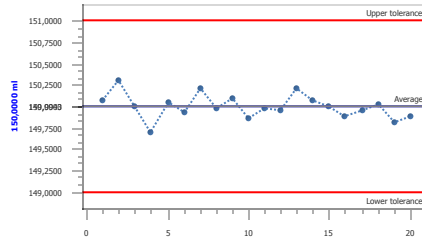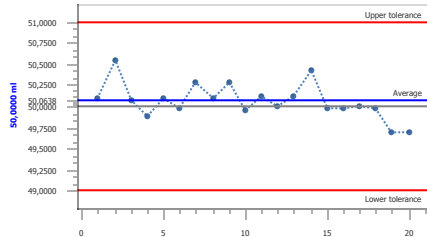

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	44
Date:	18.06.2018
Balance:	Sartorius - LA 1200 S

