

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 100 BL

**Grad. cylinder, 1000:10 ml, blue grad., A, conf. cert.**




**Batch:** 38-21

**Serial:**

**Measuring Nr.:** 49348

**Batch size:** 150

Volume:	200,000 ml	600,000 ml	1000,000 ml
<b>Tolerance:</b>	± 5,0000 ml	± 5,0000 ml	± 5,0000 ml
<b>Average value:</b>	198,9723 ml	600,0064 ml	1000,5416 ml
<b>Deviation:</b>	0,6160 ml	0,8229 ml	0,6938 ml
<b>Precision (CV):</b>	0,3080 %	0,1372 %	0,0694 %

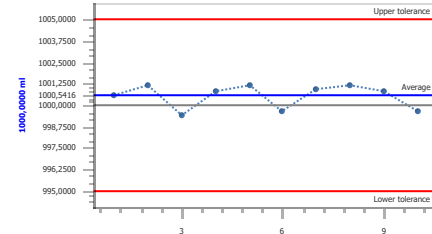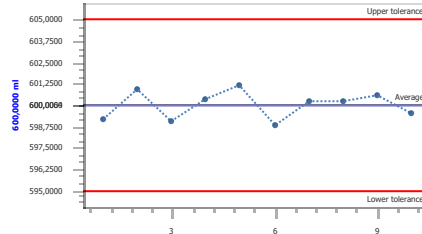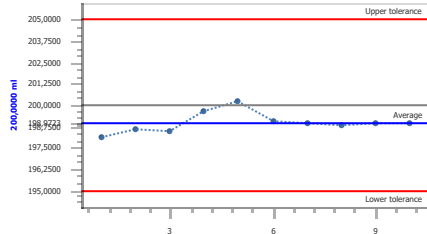

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	29.09.2021
<b>Balance:</b>	Sartorius - LC 6200 S

