

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 100 USP

Graduated cylinder, 1000 ml, USP, A, conf. cert.




Batch: 11-22

Serial:

Measuring Nr. 53119

Batch size: 150

Volume:	200,000 ml	600,000 ml	1000,000 ml
Tolerance:	± 3,0000 ml	± 3,0000 ml	± 3,0000 ml
Average value:	199,8715 ml	600,0934 ml	1001,0256 ml
Deviation:	0,4108 ml	0,7147 ml	0,5364 ml
Precision (CV):	0,2054 %	0,1191 %	0,0536 %

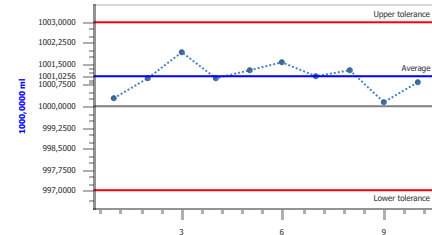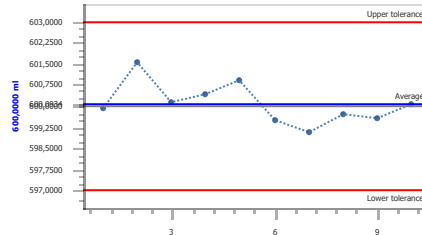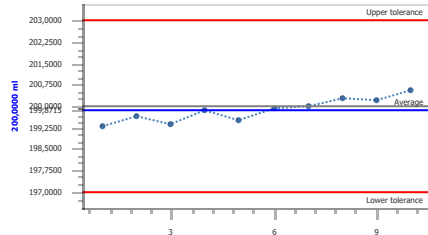

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	18.03.2022
Balance:	Sartorius - LC 6200 S

