

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 100 USP

Graduated cylinder, 1000 ml, USP, A, conf. cert.




Batch: 49-24

Serial:

Measuring Nr.: 71188

Batch size: 175

Volume:	200,000 ml	600,000 ml	1000,000 ml
Tolerance:	± 3,0000 ml	± 3,0000 ml	± 3,0000 ml
Average value:	200,4698 ml	600,0552 ml	1000,0736 ml
Deviation:	0,6281 ml	0,6176 ml	0,4130 ml
Precision (CV):	0,3140 %	0,1029 %	0,0413 %

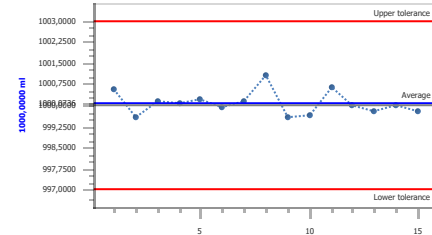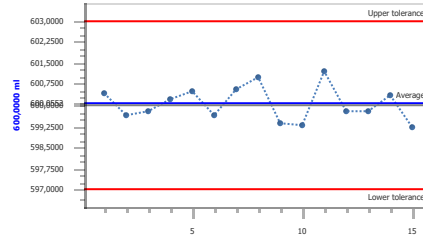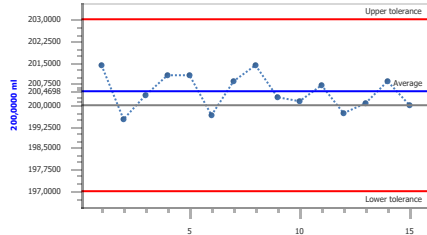

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	11.12.2024
Balance:	Sartorius - MSE14202S- OCE-D0

