

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 100

Graduated cylinder, 1000:10 ml, A, conf. cert.




Batch: 37-17

Serial:

Measuring Nr. 14119

Batch size: 793

Volume:	200,000 ml	600,000 ml	1000,000 ml
Tolerance:	± 5,0000 ml	± 5,0000 ml	± 5,0000 ml
Average value:	200,3114 ml	600,1626 ml	999,6775 ml
Deviation:	0,7589 ml	0,4824 ml	0,8433 ml
Precision (CV):	0,3795 %	0,0804 %	0,0843 %

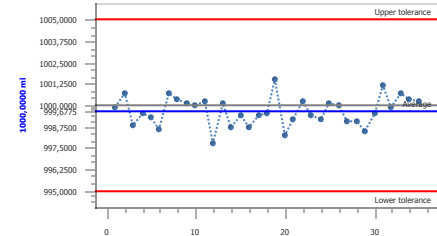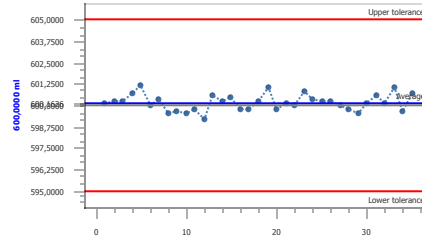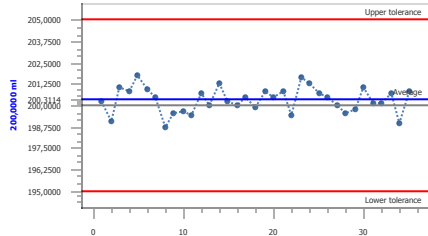

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	15.09.2017
Balance:	Sartorius - LC 6200 S

