

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 200 BL

Grad. cylinder, 2000:20 ml, blue grad., A, conf. cert.




Batch: 04-24

Serial:

Measuring Nr. 65863

Batch size: 50

Volume:	400,000 ml	1200,000 ml	2000,000 ml
Tolerance:	± 10,000 ml	± 10,000 ml	± 10,000 ml
Average value:	399,1143 ml	1199,0203 ml	1999,0125 ml
Deviation:	0,5694 ml	0,9054 ml	0,7736 ml
Precision (CV):	0,1423 %	0,0754 %	0,0387 %

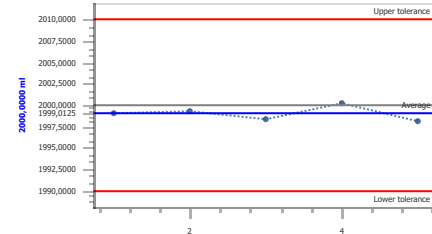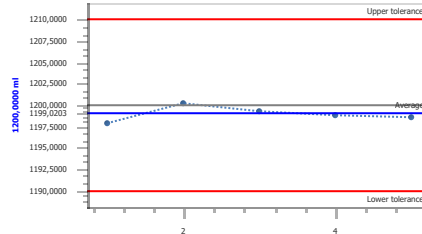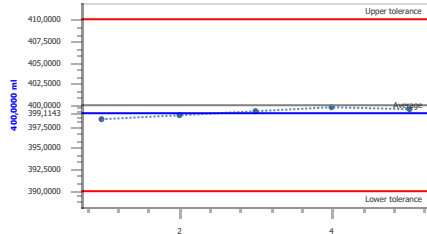

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	29.01.2024
Balance:	Sartorius - MSE14202S- OCE-D0

