

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 200

Graduated cylinder, 2000:20 ml, A, conf. cert.




Batch: 05-19

Serial:

Measuring Nr.: 27460

Batch size: 142

Volume:	400,000 ml	1200,000 ml	2000,000 ml
Tolerance:	± 10,000 ml	± 10,000 ml	± 10,000 ml
Average value:	401,3543 ml	1201,0586 ml	2000,2412 ml
Deviation:	1,1586 ml	0,9546 ml	0,7030 ml
Precision (CV):	0,2896 %	0,0795 %	0,0351 %

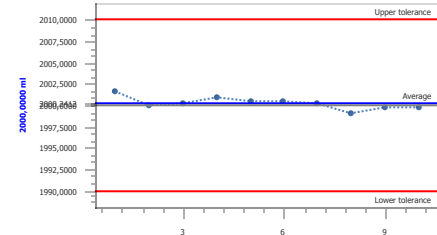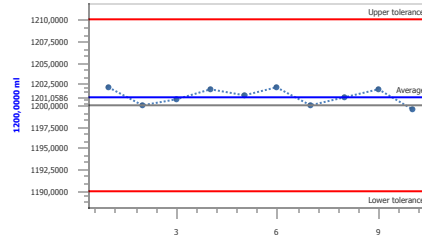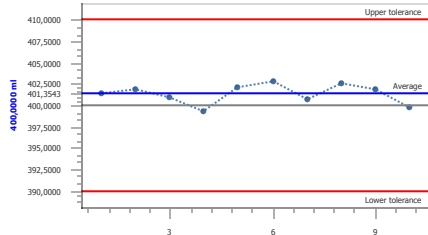

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	04.02.2019
Balance:	Sartorius - MSE14202S- OCE-D0

