

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 754 005

Grad. cylinder, 50:1 ml, NS 19, A, conf. cert.




Batch: 48-18

Serial:

Measuring Nr. 26477

Batch size: 228

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	10,1004 ml	30,0717 ml	50,0441 ml
Deviation:	0,0767 ml	0,0424 ml	0,0290 ml
Precision (CV):	0,7668 %	0,1413 %	0,0579 %

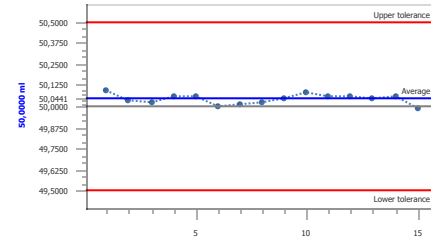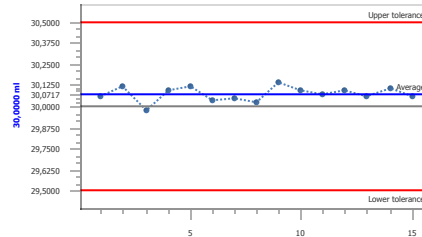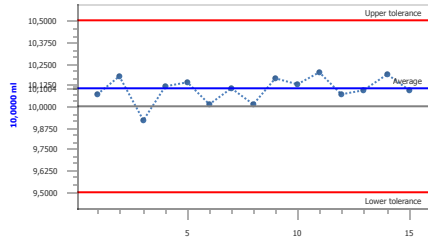

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	13.12.2018
Balance:	Sartorius - LE244S-OCE

