

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 754 010

Grad. cylinders, 100:1 ml, NS 24, A, conf. cert.




Batch: 26-18

Serial:

Measuring Nr. 21854

Batch size: 267

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	20,0319 ml	60,0581 ml	100,0744 ml
Deviation:	0,1179 ml	0,0750 ml	0,0657 ml
Precision (CV):	0,5896 %	0,1251 %	0,0657 %

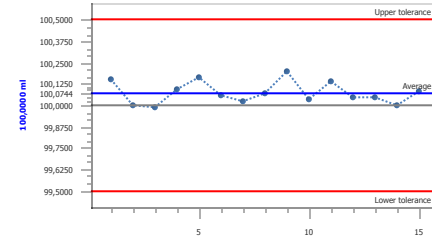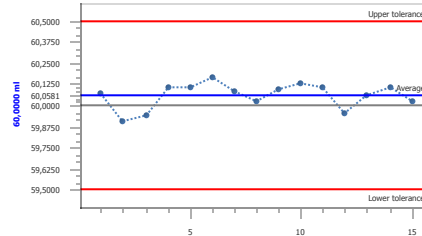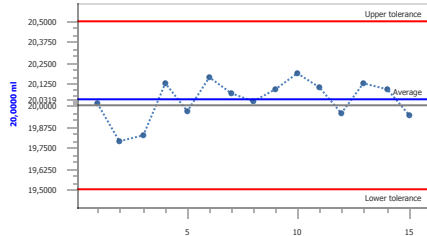

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	29.06.2018
Balance:	Sartorius - LE244S-OCE

