

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 754 025

Graduated cylinder, 250:2 ml, NS 29, A, KB




Batch: 43-19

Serial:

Measuring Nr. 34040

Batch size: 58

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
Average value:	49,7733 ml	149,9712 ml	250,0607 ml
Deviation:	0,2667 ml	0,2299 ml	0,1520 ml
Precision (CV):	0,5334 %	0,1533 %	0,0608 %

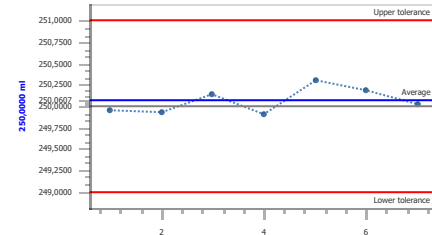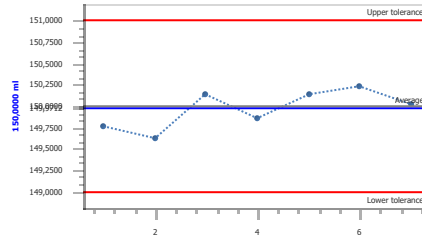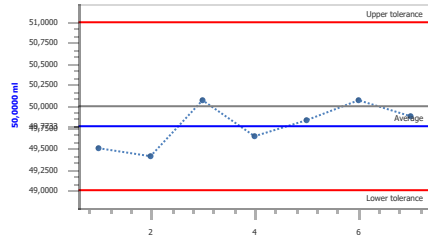

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	31.10.2019
Balance:	Sartorius - LA 1200 S

