

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 754 100

Grad. cylinder, 1000 ml, NS 45, A, conf. cert.




Batch: 26-23

Serial:

Measuring Nr. 63591

Batch size: 70

Volume:	200,000 ml	600,000 ml	1000,000 ml
Tolerance:	± 5,0000 ml	± 5,0000 ml	± 5,0000 ml
Average value:	200,2300 ml	600,7947 ml	1000,8432 ml
Deviation:	0,3684 ml	0,3691 ml	0,3917 ml
Precision (CV):	0,1842 %	0,0615 %	0,0392 %

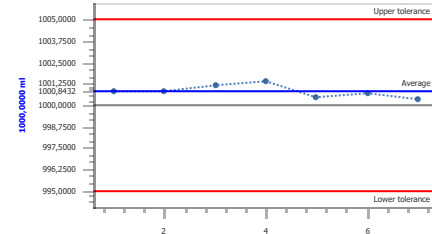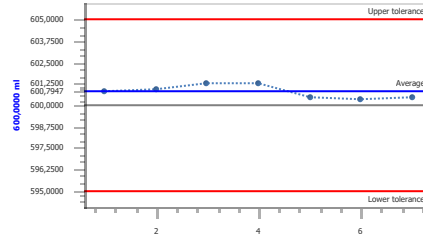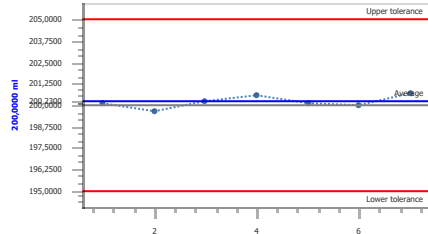

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	03.07.2023
Balance:	Sartorius - MSE14202S- OCE-D0

