

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 002 BL USP

Vol. flasks, 20 ml, NS 10, blue grad., USP, A, conf. cert.


Batch: 27-19

Serial:

Measuring Nr. 31227

Batch size: 500

Volume:	20,000 ml
Tolerance:	$\pm 0,0300$ ml
Average value:	20,0047 ml
Deviation:	0,0068 ml
Precision (CV):	0,0338 %

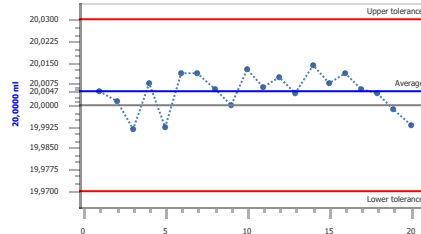

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	04.07.2019
Balance:	Sartorius - LE244S-OCE

DE-M