

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 002 BL USP

Vol. flasks, 20 ml, NS 10, blue grad., USP, A, conf. cert.


Batch: 31-22

Serial:

Measuring Nr. 58708

Batch size: 280

Volume:	20,000 ml
Tolerance:	$\pm 0,0300$ ml
Average value:	20,0171 ml
Deviation:	0,0044 ml
Precision (CV):	0,0219 %

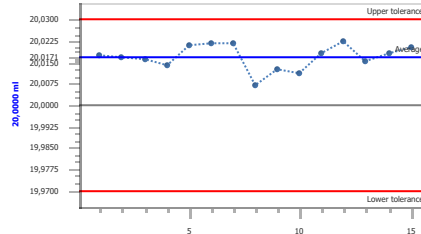

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	07.09.2022
Balance:	Sartorius - MSE224S-0CE -DU

DE-M