

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 006 USP

Volumetric flask, 50 ml, NS 14, A, USP, conf. cert.,


Batch: 18-19

Serial:

Measuring Nr. 30210

Batch size: 86

Volume:	50,0000 ml
Tolerance:	± 0,0800 ml
Average value:	49,9922 ml
Deviation:	0,0068 ml
Precision (CV):	0,0135 %

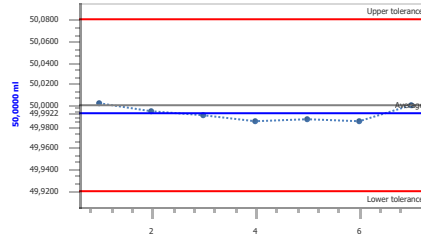

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	28.05.2019
Balance:	Sartorius - LE244S-OCE

DE-M