

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 662 010

**Volumetric flask, 100 ml, NS 12, A, conf. cert.**


**Batch:** 27-20

**Serial:**

**Measuring Nr.** 39106

**Batch size:** 3195

|                        |                   |
|------------------------|-------------------|
| <b>Volume:</b>         | <b>100,000 ml</b> |
| <b>Tolerance:</b>      | $\pm 0,1000$ ml   |
| <b>Average value:</b>  | 100,0049 ml       |
| <b>Deviation:</b>      | 0,0202 ml         |
| <b>Precision (CV):</b> | 0,0202 %          |

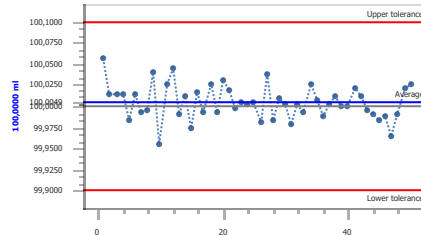

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|                  |                                   |
|------------------|-----------------------------------|
| <b>Operator:</b> | 7                                 |
| <b>Date:</b>     | 15.07.2020                        |
| <b>Balance:</b>  | Sartorius -<br>MSE224S-0CE<br>-DU |

DE-M