

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 011

Volumetric flask, 100 ml, NS 14, A, conf. cert.


Batch: 21-20

Serial:

Measuring Nr. 38465

Batch size: 3144

| | |
|------------------------|-------------------|
| Volume: | 100,000 ml |
| Tolerance: | $\pm 0,1000$ ml |
| Average value: | 99,9906 ml |
| Deviation: | 0,0128 ml |
| Precision (CV): | 0,0128 % |

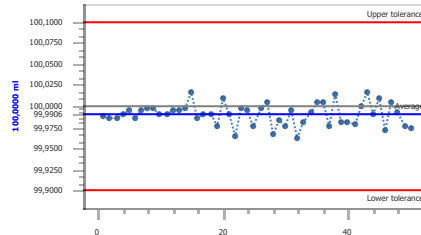

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|-----------------------------------|
| Operator: | 7 |
| Date: | 08.06.2020 |
| Balance: | Sartorius - MSE224S-0CE -DU |

DE-M