

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 012 BL USP

Vol. flask, 10 ml, NS 10, blue grad., USP, A, conf. cert.


Batch: 04-19

Serial:

Measuring Nr. 27018

Batch size: 498

Volume:	10,0000 ml
Tolerance:	$\pm 0,0200$ ml
Average value:	9,9990 ml
Deviation:	0,0042 ml
Precision (CV):	0,0417 %

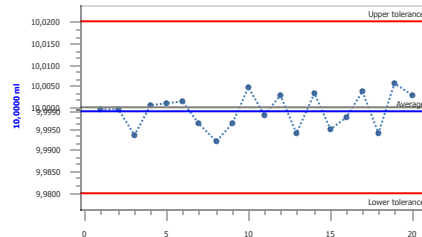

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator: 9

Date: 25.01.2019

Balance: Sartorius -
LE244S-OCE

DE-M