

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 012 BL USP

Vol. flask, 10 ml, NS 10, blue grad., USP, A, conf. cert.

Batch: 43-24


Serial:

Measuring Nr. 69801

Batch size:

279

Volume:	10,0000 ml
Tolerance:	$\pm 0,0200$ ml
Average value:	10,0019 ml
Deviation:	0,0060 ml
Precision (CV):	0,0603 %

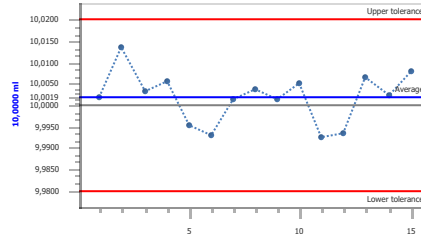

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

26.10.2024

Balance:

Sartorius -
MSE224S-0CE
-DU

DE-M