

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 013 BL

Vol. flasks, 20 ml, NS 12, blue grad., A, conf. cert.


Batch: 43-20

Serial:

Measuring Nr. 41714

Batch size: 1199

| | |
|------------------------|-----------------|
| Volume: | 20,000 ml |
| Tolerance: | $\pm 0,0600$ ml |
| Average value: | 20,0021 ml |
| Deviation: | 0,0059 ml |
| Precision (CV): | 0,0297 % |

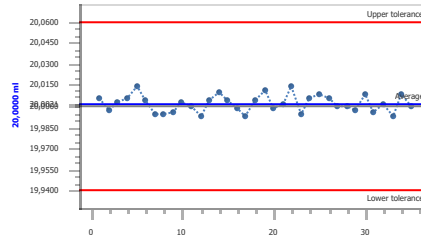

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|-----------------------------------|
| Operator: | 4 |
| Date: | 27.10.2020 |
| Balance: | Sartorius - MSE224S-0CE -DU |

DE-M