

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 014 BL

Vol. flasks, 25 ml, NS 12, blue grad., A, conf. cert.

Batch: 03-20


Serial:

Measuring Nr. 35696

Batch size:

1191

Volume:	25,0000 ml
Tolerance:	$\pm 0,0600$ ml
Average value:	25,0073 ml
Deviation:	0,0168 ml
Precision (CV):	0,0673 %

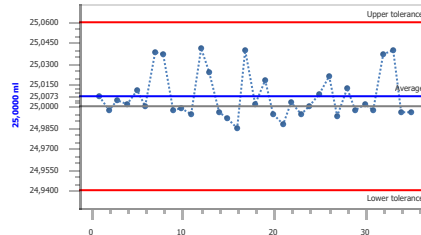

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

24.01.2020

Balance:

Sartorius -
MSE224S-0CE
-DU

DE-M