

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 015 BL USP

Vol. flasks, 5 ml, NS 10, blue grad., USP, A, conf. cert.

Batch: 22-24


Serial:

Measuring Nr. 67401

Batch size:

149

Volume:	5,0000 ml
Tolerance:	$\pm 0,0200$ ml
Average value:	4,9981 ml
Deviation:	0,0020 ml
Precision (CV):	0,0394 %

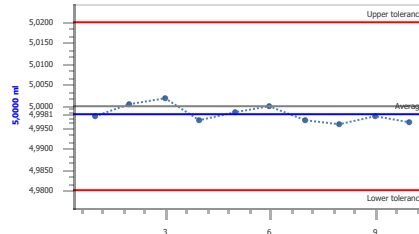

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

07.06.2024

Balance:

Sartorius -
LE244S-OCE

DE-M