


Certificate of performance

Article number 3 662 015 USP
Batch 05-17
Serial number
Measuringnr./Batch size 10073 / 87
Balance Sartorius - LE244S-0CE
Operator 4
Date 02.02.2017

Volumetric flask 5 ml NS 10 USP

Volume 5,0000ml
Tolerance 0,0200ml
Average volume 4,9997 ml
Deviation 0,0045 ml
Number of measurings 7

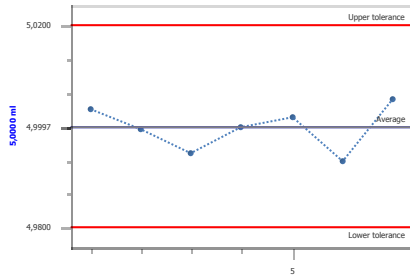

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
| info@witeg.de



ISO 9001
CERTIFIED

