

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 020 BL

Vol. flasks, 200 ml, NS 14, blue grad., A, conf. cert.


Batch: 06-18

Serial:

Measuring Nr. 19027

Batch size: 240

Volume:	200,000 ml
Tolerance:	$\pm 0,1500$ ml
Average value:	200,0109 ml
Deviation:	0,0224 ml
Precision (CV):	0,0112 %

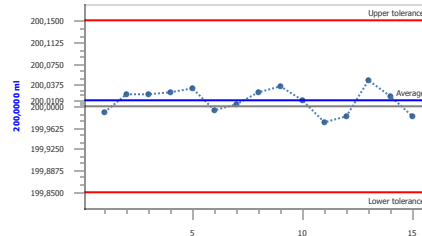

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator: 4

Date: 21.03.2018

Balance: Sartorius - LA
1200 S

DE-M