

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 020 BL

Vol. flask, 200 ml, NS 14, blue grad., A, conf. cert.

Batch: 34-19


Serial:

Measuring Nr. 32801

Batch size:

1200

| | |
|------------------------|-----------------|
| Volume: | 200,000 ml |
| Tolerance: | $\pm 0,1500$ ml |
| Average value: | 200,0118 ml |
| Deviation: | 0,0259 ml |
| Precision (CV): | 0,0129 % |

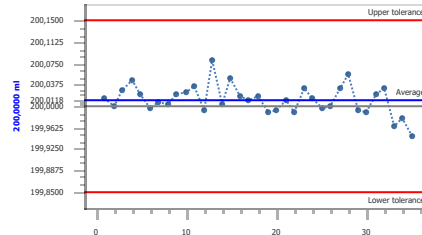

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

05.09.2019

Balance:

Sartorius - LA
1200 S

DE-M