

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 020

Volumetric flask, 200 ml, NS 14, A, conf. cert.


Batch: 22-22

Serial:

Measuring Nr. 56513

Batch size: 1200

| | |
|------------------------|-----------------|
| Volume: | 200,000 ml |
| Tolerance: | $\pm 0,1500$ ml |
| Average value: | 200,0016 ml |
| Deviation: | 0,0215 ml |
| Precision (CV): | 0,0107 % |

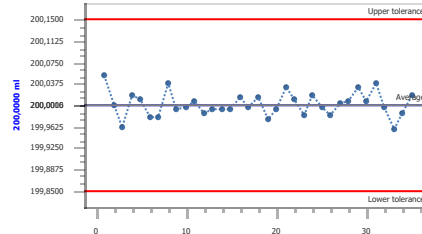

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|--------------------------|
| Operator: | 4 |
| Date: | 09.06.2022 |
| Balance: | Sartorius - LA 1200 S |

DE-M