

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 050 BL

Vol. flasks, 500 ml, NS 19, blue grad., A, conf. cert.


Batch: 41-17

Serial:

Measuring Nr. 15539

Batch size: 1200

Volume:	500,000 ml
Tolerance:	$\pm 0,2500$ ml
Average value:	500,0312 ml
Deviation:	0,0332 ml
Precision (CV):	0,0066 %

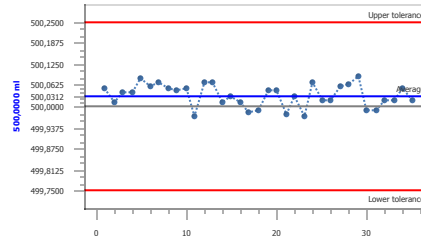

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	06.11.2017
Balance:	Sartorius - LA 1200 S

DE-M