


Certificate of performance

Article number 3 662 050 USP
Batch 08-17
Serial number
Measuringnr./Batch size 10159 / 150
Balance Sartorius - LA 1200 S
Operator 4
Date 27.02.2017

Volumetric flasks 500 ml NS 19 USP

Volume 500,0000ml
Tolerance 0,2000ml
Average volume 499,9805 ml
Deviation 0,0244 ml
Number of measurings 10

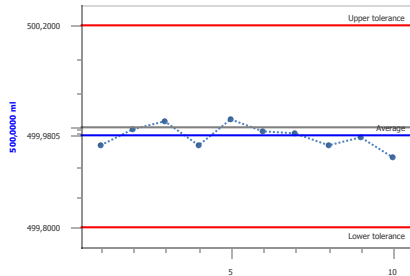

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
| info@witeg.de

