

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 662 100 USP

**Volumetric flask, 1000 ml, NS 24, USP, A, conf. cert.**


**Batch:** 08-22

**Serial:**

**Measuring Nr.** 52774

**Batch size:** 90

|                        |                    |
|------------------------|--------------------|
| <b>Volume:</b>         | <b>1000,000 ml</b> |
| <b>Tolerance:</b>      | $\pm 0,3000$ ml    |
| <b>Average value:</b>  | 1000,1291 ml       |
| <b>Deviation:</b>      | 0,0270 ml          |
| <b>Precision (CV):</b> | 0,0027 %           |

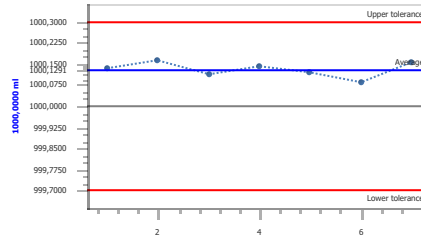

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|                  |                          |
|------------------|--------------------------|
| <b>Operator:</b> | 7                        |
| <b>Date:</b>     | 03.03.2022               |
| <b>Balance:</b>  | Sartorius - LC<br>6200 S |

DE-M