

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 101 BL

Vol. flasks, 1000 ml, NS 29, blue grad., A, conf. cert.


Batch: 15-19

Serial:

Measuring Nr. 29767

Batch size: 279

Volume:	1000,0000 ml
Tolerance:	$\pm 0,6000$ ml
Average value:	1000,0482 ml
Deviation:	0,0584 ml
Precision (CV):	0,0058 %

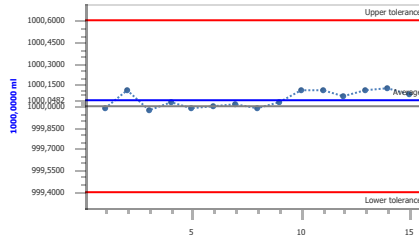

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	09.05.2019
Balance:	Sartorius - MSE14202S- OCE-D0

DE-M