

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 1500

Volumetric flask, 1500 ml, NS 29, A, conf. cert.


Batch: 03-23

Serial: -

Measuring Nr. 61112

Batch size: 2

Volume:	1500,000 ml
Tolerance:	$\pm 0,6000$ ml
Average value:	1500,2066 ml
Deviation:	0,1206 ml
Precision (CV):	0,0080 %

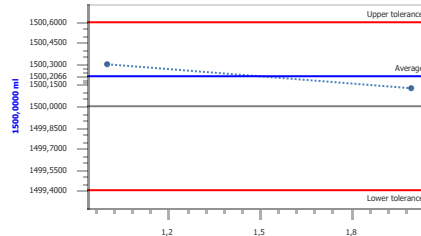

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

19.01.2023

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M