

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 192

Vol. flask, 192,2 ml, NS 14, blue grad., A, conf. cert.

Batch: 33-19


Serial:

Measuring Nr. 32232

Batch size:

15

Volume:	192,2000 ml
Tolerance:	$\pm 0,1500$ ml
Average value:	192,2970 ml
Deviation:	0,0117 ml
Precision (CV):	0,0061 %

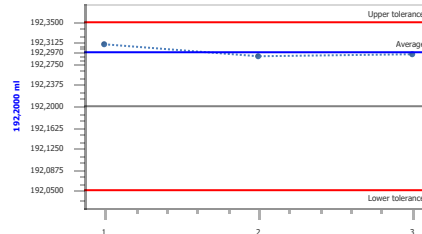

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	21.08.2019
Balance:	Sartorius - LA 1200 S

DE-M