

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 200 BL

Vol. flask, 2000 ml, NS 29, blue grad., A, conf. cert.

Batch: 25-23


Serial:

Measuring Nr. 63765

Batch size:

126

Volume:	2000,0000 ml
Tolerance:	$\pm 0,6000$ ml
Average value:	1999,9093 ml
Deviation:	0,0753 ml
Precision (CV):	0,0038 %

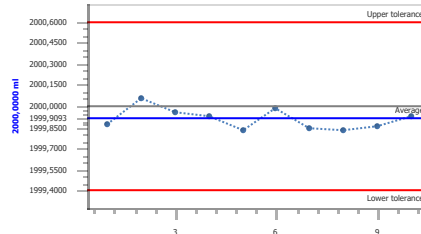

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

14.07.2023

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M