

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 400 BL

Vol. flask, 4000 ml, NS 34, blue grad., A, conf. cert.

Batch: 09-21


Serial:

Measuring Nr. 44891

Batch size:

6

Volume:	4000,0000 ml
Tolerance:	$\pm 1,2000$ ml
Average value:	4000,2271 ml
Deviation:	0,1420 ml
Precision (CV):	0,0036 %

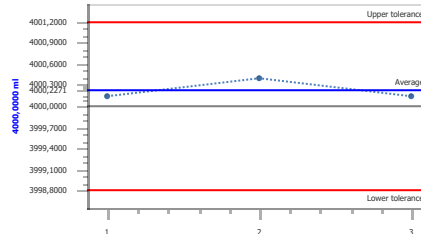

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

04.03.2021

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M