

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 500

Volumetric flask, 5000 ml, NS 34, A, conf. cert.


Batch: 19-19

Serial:

Measuring Nr. 30304

Batch size: 35

| | |
|------------------------|-----------------|
| Volume: | 5000,0000 ml |
| Tolerance: | $\pm 1,2000$ ml |
| Average value: | 5000,1770 ml |
| Deviation: | 0,2645 ml |
| Precision (CV): | 0,0053 % |

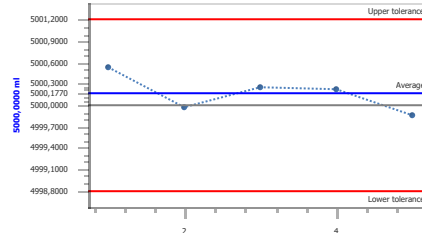

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|-------------------------------------|
| Operator: | 4 |
| Date: | 04.06.2019 |
| Balance: | Sartorius - MSE14202S- OCE-D0 |

DE-M