

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 600 BL

Volumetric flask, 6000 ml, NS 34, A, conf. cert.

Batch: 19-18


Serial:

Measuring Nr. 20769

Batch size:

4

| | |
|------------------------|-----------------|
| Volume: | 6000,0000 ml |
| Tolerance: | $\pm 1,2000$ ml |
| Average value: | 6000,6296 ml |
| Deviation: | 0,1871 ml |
| Precision (CV): | 0,0031 % |

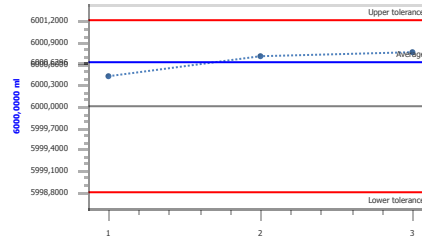

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

17.05.2018

Balance:

Precisa - 12000
SCS

DE-M