

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 669 000 BR

Vol. flasks, 1 ml, NS 7, amber glass, A, conf. cert.


Batch: 15-19

Serial:

Measuring Nr. 29264

Batch size: 280

Volume:	1,0000 ml
Tolerance:	$\pm 0,0250$ ml
Average value:	1,0036 ml
Deviation:	0,0039 ml
Precision (CV):	0,3915 %

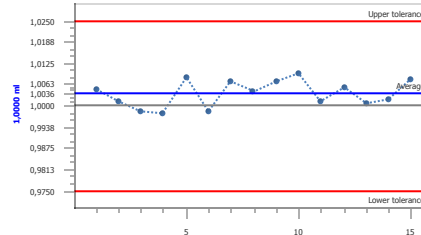

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	0
Date:	12.04.2019
Balance:	Sartorius - LE244S-OCE

DE-M