

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 010 USP

Vol. flask, 100 ml, NS 12, USP, amber gl., A, conf. cert.


Batch: 47-19

Serial:

Measuring Nr. 34772

Batch size: 150

Volume:	100,000 ml
Tolerance:	$\pm 0,0800$ ml
Average value:	99,9720 ml
Deviation:	0,0076 ml
Precision (CV):	0,0076 %

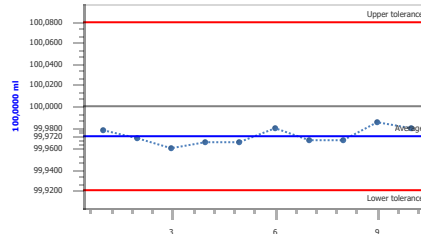

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	03.12.2019
Balance:	Sartorius - MSE224S-0CE -DU

DE-M