

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 010 USP

Vol. flask, 100 ml, NS 12, USP, amber gl., A, conf. cert.


Batch: 48-20

Serial:

Measuring Nr. 43010

Batch size: 150

| | |
|------------------------|-------------|
| Volume: | 100,000 ml |
| Tolerance: | ± 0,0800 ml |
| Average value: | 99,9889 ml |
| Deviation: | 0,0140 ml |
| Precision (CV): | 0,0140 % |

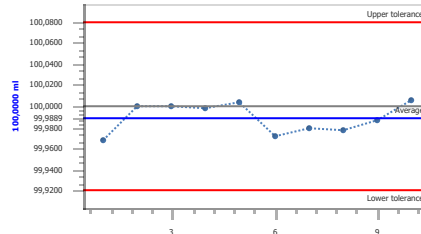

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|---------------------------|
| Operator: | 7 |
| Date: | 04.12.2020 |
| Balance: | Sartorius - LE244S-OCE |

DE-M