

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 013

Vol. flasks, 20 ml, NS 12, amber glass, A, conf. cert.

Batch: 30-20


Serial:

Measuring Nr. 39391

Batch size:

500

| | |
|------------------------|-----------------|
| Volume: | 20,000 ml |
| Tolerance: | $\pm 0,0600$ ml |
| Average value: | 20,0012 ml |
| Deviation: | 0,0119 ml |
| Precision (CV): | 0,0595 % |

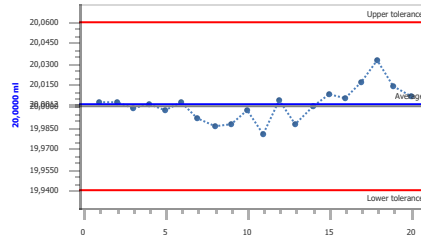

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

9

Date:

05.08.2020

Balance:

Sartorius -
LE244S-OCE

DE-M