

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 670 015 USP

**Vol. flasks, 5 ml, NS 10, amber glass, USP, conf. cert.**

**Batch:** 43-18


**Serial:**

**Measuring Nr.** 25423

**Batch size:**

180

<b>Volume:</b>	5,0000 ml
<b>Tolerance:</b>	$\pm 0,0200$ ml
<b>Average value:</b>	4,9980 ml
<b>Deviation:</b>	0,0065 ml
<b>Precision (CV):</b>	0,1301 %

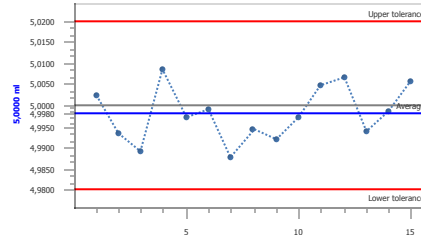

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:** 9

**Date:** 06.11.2018

**Balance:** Sartorius -  
LE244S-OCE

DE-M