

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 670 025

**Vol. flask, 250 ml, NS 14, amber glass, A, conf. cert.**

**Batch:** 04-20


**Serial:**

**Measuring Nr.** 35846

**Batch size:**

1196

<b>Volume:</b>	<b>250,000 ml</b>
<b>Tolerance:</b>	$\pm 0,1500$ ml
<b>Average value:</b>	249,9899 ml
<b>Deviation:</b>	0,0516 ml
<b>Precision (CV):</b>	0,0207 %

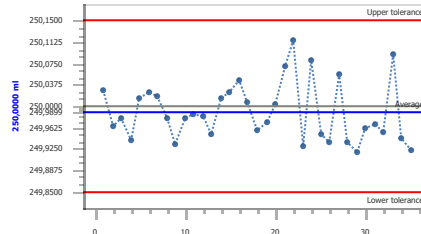

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

4

**Date:**

05.02.2020

**Balance:**

Sartorius - LA  
1200 S

DE-M