

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 050 USP

Vol. flask, 500 ml, NS 19, USP, amber, A, conf. cert.


Batch: 07-23

Serial:

Measuring Nr. 61785

Batch size: 149

Volume:	500,000 ml
Tolerance:	$\pm 0,2000$ ml
Average value:	499,9906 ml
Deviation:	0,0209 ml
Precision (CV):	0,0042 %

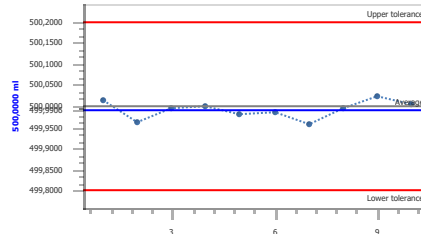

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	21.02.2023
Balance:	Sartorius - LE244S-OCE

DE-M