

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 670 050

**Vol. flasks, 500 ml, NS 19, amber glass, A, conf. cert.**


**Batch:** 41-17

**Serial:**

**Measuring Nr.** 15374

**Batch size:** 280

<b>Volume:</b>	<b>500,000 ml</b>
<b>Tolerance:</b>	$\pm 0,2500$ ml
<b>Average value:</b>	500,1313 ml
<b>Deviation:</b>	0,0480 ml
<b>Precision (CV):</b>	0,0096 %

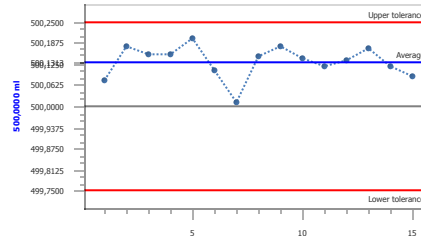

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	24.10.2017
<b>Balance:</b>	Sartorius - LA 1200 S

DE-M