

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 100 USP

Vol. flask, 1000 ml, NS 24, amber gl., USP, A, conf. cert.

Batch: 44-21


Serial:

Measuring Nr. 50459

Batch size:

56

Volume:	1000,0000 ml
Tolerance:	$\pm 0,3000$ ml
Average value:	999,9778 ml
Deviation:	0,0925 ml
Precision (CV):	0,0092 %

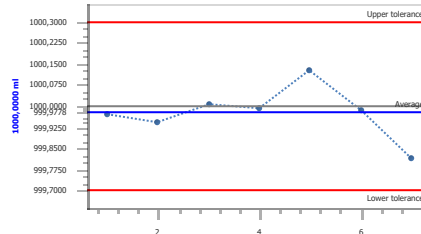

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

15.11.2021

Balance:

Sartorius - LC
6200 S

DE-M