

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 100

Vol. flask, 1000 ml, NS 24, amber glass, A, conf. cert.


Batch: 50-19

Serial:

Measuring Nr. 35185

Batch size: 54

| | |
|------------------------|--------------------|
| Volume: | 1000,000 ml |
| Tolerance: | $\pm 0,4000$ ml |
| Average value: | 999,9878 ml |
| Deviation: | 0,0854 ml |
| Precision (CV): | 0,0085 % |

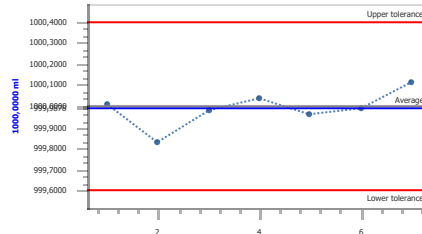

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|--------------------------|
| Operator: | 4 |
| Date: | 12.12.2019 |
| Balance: | Sartorius - LC 6200 S |

DE-M