

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 100

Vol. flask, 1000 ml, NS 24, amber glass, A, conf. cert.

Batch: 04-20

Serial:

Measuring Nr. 35770

Batch size:

271


Volume: 1000,0000 ml

Tolerance: $\pm 0,4000$ ml

Average value: 999,9898 ml

Deviation: 0,1057 ml

Precision (CV): 0,0106 %

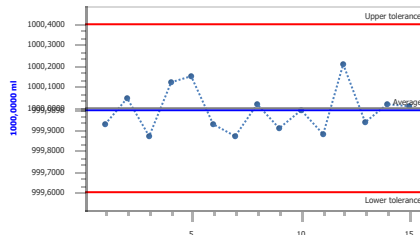

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

29.01.2020

Balance:

Sartorius - LC
6200 S

DE-M