

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 500

Vol. flask, 5000 ml, NS 34, amber glass, A, conf. cert.


Batch: 23-20

Serial:

Measuring Nr. 38356

Batch size: 20

Volume:	5000,0000 ml
Tolerance:	± 1,2000 ml
Average value:	5000,3084 ml
Deviation:	0,1160 ml
Precision (CV):	0,0023 %

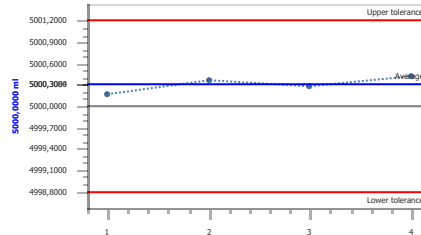

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	03.06.2020
Balance:	Sartorius - MSE14202S- OCE-D0

DE-M