

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 500

Vol. flask, 5000 ml, NS 34, amber glass, A, conf. cert.

Batch: 49-20


Serial:

Measuring Nr. 43046

Batch size:

10

| | |
|------------------------|-----------------|
| Volume: | 5000,0000 ml |
| Tolerance: | $\pm 1,2000$ ml |
| Average value: | 4999,7543 ml |
| Deviation: | 0,2018 ml |
| Precision (CV): | 0,0040 % |

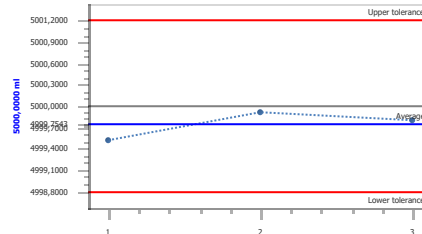

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

07.12.2020

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M